


TECHNICAL DATA-SHEET

X-RAY FILM VIEWER FOR MAMMOGRAPHY HIGH LIGHT INTENSITY

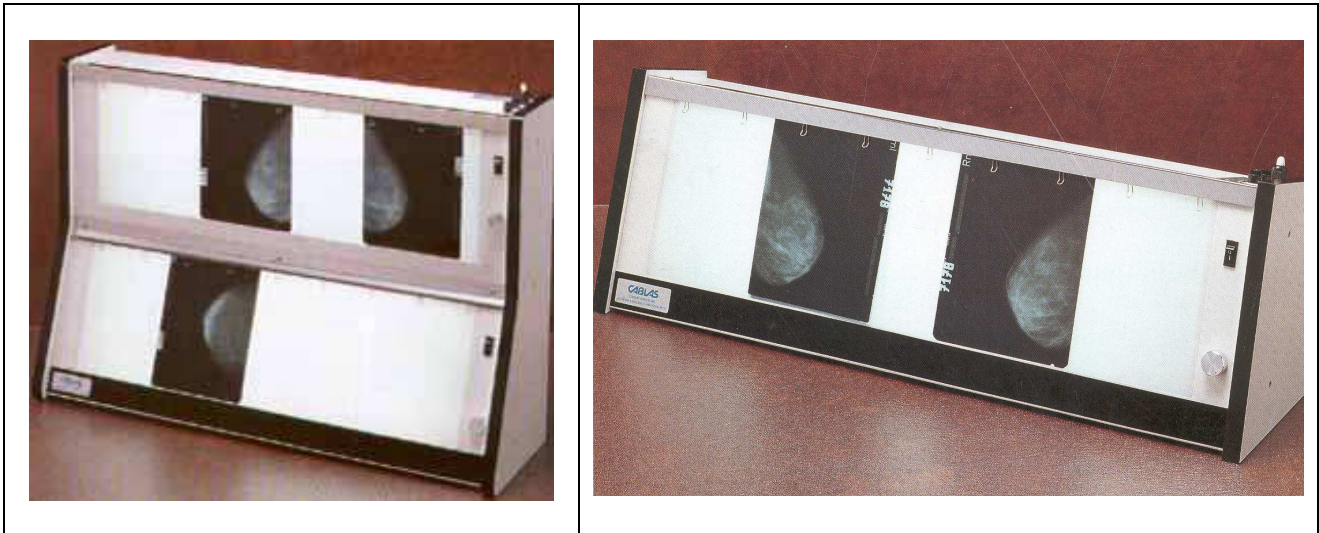

- Stove enamelled steel structure 0,8 mm;
- Fire epoxy painting colour peel RAL 9010, upon structure cleaning treatment;
- Neon tubes 6.000°K ((other type of tubes available on request);
- Speed switching;
- Light regulator which allows a very good light regulation from 100% al 10%;
- Upper and/or central pressing rolls film holding system;
- Speed bipolar switch on the front (on request is possible to apply other type and/or their position);
- External fuses lagging type 5x20 (positioned on the bottom right side);
- Feeling cable with schuko plug CE 3 0,75;
- Predisposed for wall installation through expansion dowels;
- X-ray film viewer conforms to Directive 93/42/CEE - Medical Devices - Class 1

Moreover meets the Directive 73/23 CEE (Low tension)

89/336 CEE (Electromagnetic compatibility)

The construction conforms to Norms EN 60601 -1,2 - Din 6856 -1,2;

- Can be installed in rooms as medical use (CEI 64-4);
- Feeding 230V / 50Hz;
- Maintenance : recurrent cleaning (each 6 months) of the whole screen and tubes replacement each 5.000 hours of use;

TECHNICAL DATA - SHEET

ONE SECTION LIGHT

CODE	FORMATO	MISURE ESTERNE	PESO	NUMERO LAMPADIE	SEZIONI LUCE	W	A	FUSIBILI	CD/MQ
M-NM-01	72 X 24	95 X 33 X 21	12	4 – 30 W	1 – 72 X 24	150	0,7	1	7300
M-NM-02	96 X 30	124 X 39 X 24	18	4 – 36 W	1 – 96 X 30	180	0,9	1	7300

TWO SECTIONS LIGHT

M-NM-03	72 X 24 X 2	95 X 63 X 21	23	8 – 30 W	2 – 72 X 24	300	1,4	2	7300
M-NM-04	96 X 30 X 2	124 X 74 X 24	32	8 – 36 W	2 – 96 X 30	360	1,6	2	7300